


Mobile Precision Smart Sensor Interface

For Load Cells, Torque and Displacement Sensors

Code: 7160 EN
Delivery: ex stock
Warranty: 24 months

Series 7160

Accuracy 0.02 %
of reading

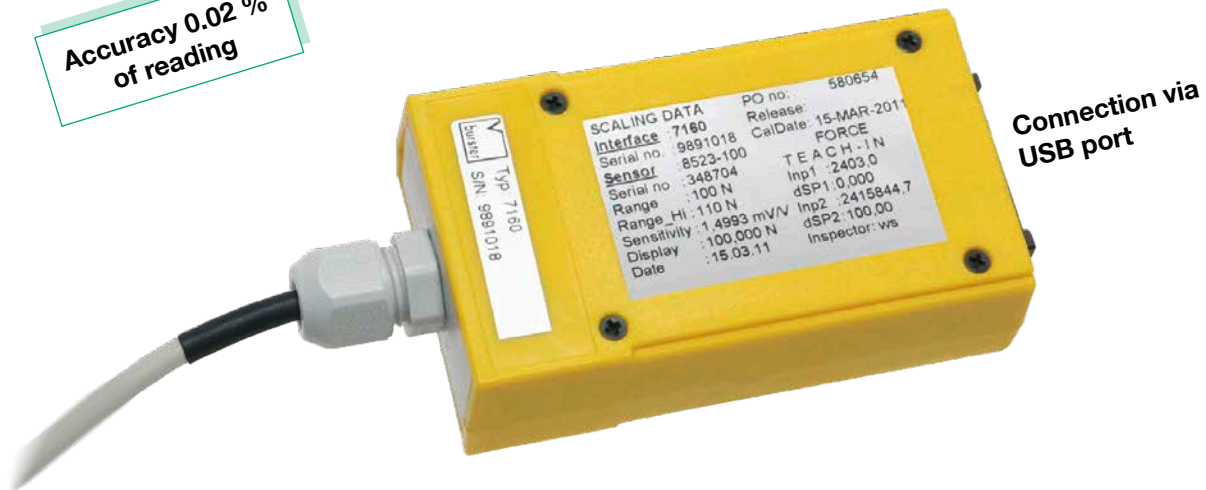

Connection via
USB port

7160 EN

- Interface for strain gauge and potentiometric sensors with "Plug & Measure" connection
- Accuracy 0.02 % of reading
- Connection system 6 wire
- User-friendly configuration and data logging software DigiCal
- DLL, LabView driver for integration into own industrial environment
- Universal reference measurement chain with DKD/DAkkS (Calibration according to German Accreditation Body) or factory calibration certificate (option)

Application

In practice it is often necessary, to acquire a sensor's measurement results nearby fast and simple. With interface model 7160 and USB adapter model 7131 the measured values of a sensor can be transmitted directly to a PC. In addition Smart Sensor Interface model 7160 can be used along with DIGISTANT® model 4423 for on-site calibration.

Application / examples:


- ▶ Calibration of testing machines
- ▶ On-site calibration of high-precision measurement equipment
- ▶ Testing hydraulic presses
- ▶ Reference measurements on/in assembly lines
- ▶ Testing robot pressing forces
- ▶ Testing compressive force on pneumatic units

Description

Smart Sensor Interface model 7160 prepares the sensor signal for the PC or for DIGISTANT® model 4423. Force, torque and displacement sensors can be connected to model 7160. Using the adapter model 7130, the measurement values can be displayed directly on model DIGISTANT® 4423. Adapter model 7131 USB transfers the measurement values directly to a PC. The entry of the sensor data is done by burster company setting and via Plug & Measure connection the sensor data are detected automatically. For each measurement the customer can choose between two operating modes. A static measuring rate and average mode reach a very high measurement accuracy. The dynamic measuring rate at 1000/sec allows the detection of peak values at reduced accuracy.

Application

Construction of a Force Measurement Chain Directly to a USB Port




Prüfprotokoll 7160-ABG
Test Certificate 7160-ABG

Smart Sensor Interface		Smart Sensor Interface	
Type	7160	PC no.	90082
Serial No.	1789900	Software release	06.03.2012
Calibration date	06.03.2012	Safety check according to DIN EN 61010-1, IEC 1010-1	
Sicherheitsprüfung nach		Quality Inspections	
Das Gerät wurde werkseitig wie folgt kalibriert:		The device was scaled as follows:	
Aufgabe-Nr.		PC no.	90082
Sensor-Bezeichnung	FORCE	Sensor Designation	FORCE
Sensor-Typ	8520-0905	Sensor Type	8520-0905
Sensor-Serien-Nr.	371646	Sensor Serial no.	371646
Messbereich	5 kN	Measuring range	5 kN
Kennwert	0,001 mN/V	Sensitivity	0,001 mN/V
Anzeige	5.000 kN @ 100 %	Display	5.000 kN @ 100 %
Faktor für Spezialeinheit	1,00 g	Factor for special unit	1,00 g
Bereichsgrenze	-50 ... 5,5 kN	Range Limits	-50 ... 5,5 kN
Unterer Engpasswert - Anzeigewert 1	Input - display cal_low - 787,0 Digit / 0,000 kN		
Oberer Engpasswert - Anzeigewert 2	Input - display cal_high - 1604367,5 Digit / 5,000 kN		
Hilfsfunktionswert - Taste-Wert	2 Zero / Zero value	0,000	0,000
Parameter: Messmodus / Messrate / Mittelwerte	Mode / Rate / AVG	STAT 3s / 8s	
Validiert nach Prüfanweisung	Validated according to Inspection instruction	1803	
Die Rückführbarkeit der verwendeten Sekundärnormale auf nationale bzw. internationale Normale, entsprechend der Normreihe DIN EN ISO 9000 ff. ist über Kalibrier- oder Eichscheme gewährleistet. Die verwendeten Normale sind auf Kalibrierstationen rückführbar, die nach ISO/IEC 17025 akkreditiert sind.			
The traceability of the used secondary standards to the national respectively international standards, according to DIN EN ISO 9000 ff. is guaranteed by Calibration Certificate. The used standards are traceable to calibration laboratories, which are accredited to ISO/IEC 17025.			
Prüfmitr.-	Typ	Hersteller	bestimmende Stelle
Equipment-No.	Type	Manufacturer	Calibration mark
716-0500-21	8505	burster	DKD-DAkkS 7700
716-0505-26	8405	burster	DKD-DAkkS 01-01
Date of Calibration: 25.11.11			
Date of Calibration: 07.03.12			
Das Gerät erfüllt die Spezifikationen. / The device performs the specifications.			
Nach der vorliegenden Erfahrung ist es empfehlenswert, das Produkt im Abstand von etwa 24 Monaten neu zu kalibrieren. / According to our experience it is recommended to recalibrate this product in intervals of 24 months.			
Raumtemperatur / Ambient temperature: 22 °C ± 0,3 K Rel. Feuchte / Relative humidity: 50 % ± 20 %			
Protokoll / Test Date: 14.03.12		Prüfer / Inspector: W. Schulte	

Application

Torque Wrench Calibration with Torque Sensor and Smart Sensor Interface 7160 and Universal Calibrator 4423




Along with the Smart Sensor Interface model 7160 torque sensors can be directly connected to the DIGISTANT® model 4423. This measuring chain allows a fast and easy measurement of torque of all tools in screw-in technology. Through on-site calibration e.g. torque wrenches can be checked for their compliance with the adjusted scale value respectively trigger accuracy. In order to render the torque measurement chain traceable a DKD/DAkkS/Manufacturer Calibration Certificate can be supplied optionally.

Checking Press-fit Forces

A force measurement chain, consisting of a load cell and a Smart Sensor Interface model 7160/7131 and USB adapter can be connected directly to the PC. The sensor data are read out by DigiCal software, printed as a protocol and exported to Excel.


For on-site calibration the load cell is placed in line with the force flow of the press-fit measuring device. In order to render the force measurement chain traceable a DKD/DAkkS Manufacturer Calibration Certificate can be supplied optionally.

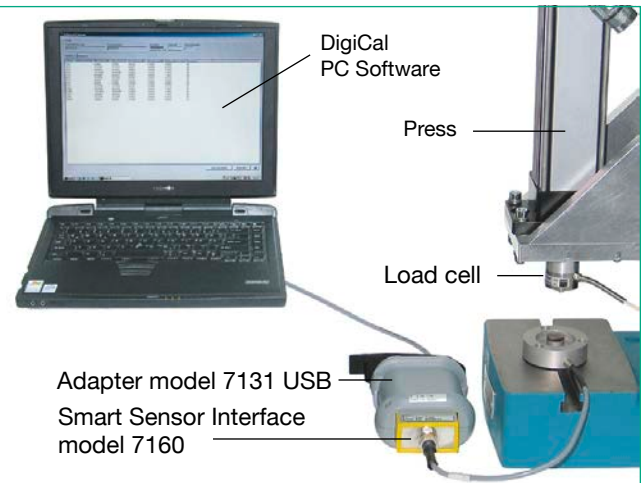

Features of Configuration and Data Logging Software DigiCal for Mechanical Values


Simple and Secure Editing of Measurement Programs and Calibration Routines

- DigiCal allows the configuration of user-friendly calibration routines through selection of physical values and measurement values to be checked. Thus a test sample can be evaluated without considerable effort for its compliance with the required technical data.
- Once created, the measurement program can be used again and again in future measurements.
- Versatile, easily selectable pop-ups allow users rapid access.

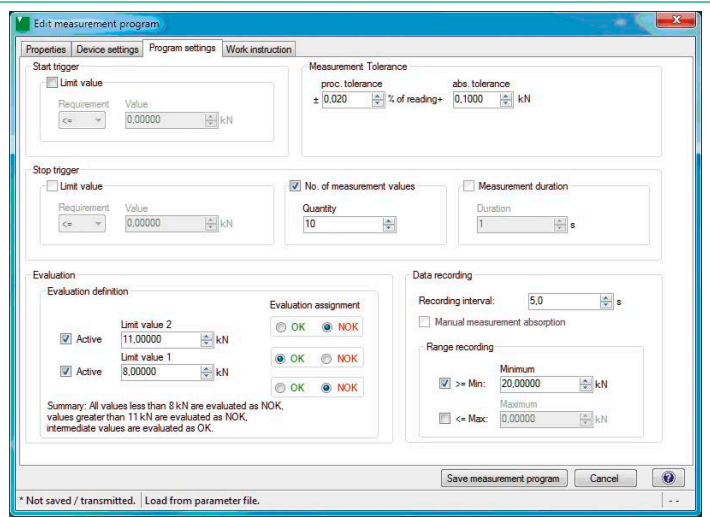

Historical Viewing of Archived Test Certificates

- History viewer allows a quick overview of the tolerance characteristics of test and measurement devices.
- Up to 4 equally measured samples of one test object can be compared. The history of the measured values identifies the stability and/or drift.

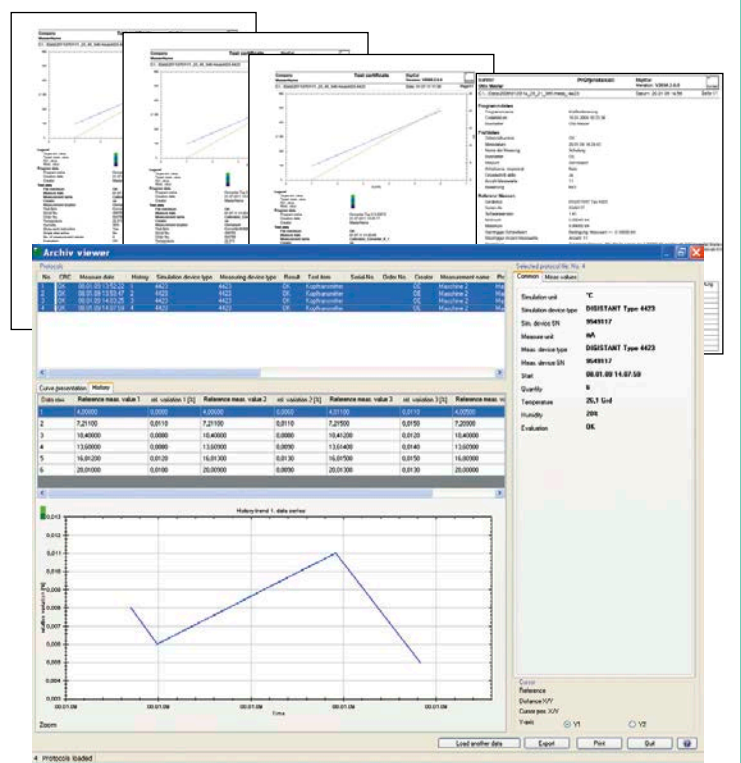

Technical Data

Connectable sensors

Strain gauge

Bridge resistance (full bridge):	350 Ω to 2000 Ω
Connection system:	6 wire
Configurable sensitivity:	± 0.5 up to ±10 mV/V
Bridge excitation:	approx. 4.5 V (is measured)
Excitation current:	max. 35 mA
Accuracy:	0.02 % of reading ± 5 μV (23 °C ± 5 °C)
Input leak current typically:	200 pA
Linearity typically:	0.0015 % F.S.
Temperature coefficient:	25 ppm/K
Noise-free resolution typically:	21 bit

Potentiometric displacement sensors

Connection system:	3 wire
Resistance range:	500 Ω up to 20 kΩ
Excitation:	approx. 4.5 V (is measured)
Excitation current:	max. 35 mA
Input leak current typically:	50 nA
Accuracy:	0.02 % of reading ± 5 μV (23 °C ± 5 °C)
Linearity typically:	0.007 % F.S.
Temperature coefficient:	25 ppm/K
Noise-free resolution typically:	23 bit

General data

Case:	synthetic material
Dimensions (W x H x D):	50 x 26 x 88 mm
Indication:	indication in DIGISTANT® 4423 via adapter 7130 or read out with PC via USB adapter model 7131-USB
Display range:	-200.000 up to 200.000 adjustable
Decimal point:	user programmable
Operating mode:	static mode dynamic maximum dynamic minimum dynamic Peak to Peak dynamic present reading
Measuring rate statically:	3/sec
Measuring rate dynamically:	adjustable from 3/sec to 1000/sec
Averaging:	X/1, X/2, X/4, X/8, X/16 and X/32
Linearization points:	2 to 21 points
Common mode:	120 dB
Limit frequency:	up to 5 KHz
Operating temperature:	0 °C up to 50 °C
Storage temperature:	-30 °C up to 60 °C

Order Information

Smart Sensor Interface for connecting force, displacement or torque sensors	Model 7160
Adapter for Smart Sensor Interface / module to DIGISTANT® model 4423	Model 7130
Adapter for Smart Sensor Interface / direct to PC via USB	Model 7131-USB
Software Configuration and data logging software DigiCal	Model 4423-P001

Ordering examples

Version adapter model 7131 USB direct to PC via USB interface with high precision load cell

Tension compression load cell	Model 8527-6020
Smart Sensor Interface for connecting force displacement or torque sensors	Model 7160
Fitting and alignment of the sensors to the Smart Sensor Interface	Model 71ABG
Adapter or Smart Sensor Interface / direct to PC via USB	Model 7131-USB
Configuration and data logging software DigiCal	Model 4423-P001
Manufacturer calibration for the complete chain, sensors, Smart Sensor Interface 7160 and software, pressure direction, 5 points in 20 % steps, rising and falling	Model 85WKS-85DXM

Version with adapter model 7130 to DIGISTANT® model 4423 with torque sensor

Torque sensor, static range 25 Nm	Model 8628-5025
Smart Sensor Interface for connecting force, displacement and torque sensors	Model 7160
Fitting and alignment of the sensors to the Smart Sensor Interface	Model 71ABG
Universal Calibrator DIGISTANT® with USB interface	Model 4423
Adapter for Smart Sensor Interface / module to DIGISTANT® model 4423	Model 7130
Configuration and data logging software DigiCal	Model 4423-P001
Manufacturer calibration for torque sensor model 8628 as chain, 20 % steps, right and left moment	Model 86WKS-LRM-5200

DKD/DAkKS Calibration Certificate

DKD/DAkKS Calibration Certificate for force up to 200 kN, pressure up to 5000 bar and torque up to 5kNm.

Manufacturer Calibration Certificate

Manufacturer Calibration Certificate for force up to 200 kN pressure up to 5000 bar, torque up to 5 kNm and displacement up to 300 mm.